

SO0001



LASER-INDUCED DAMAGE THRESHOLD (LIDT) MEASUREMENT REPORT

R-ON-1 (CONDITIONING) TEST PROCEDURE

Sample: Sample

Request from

Address	Company
	Address Line 1
	Address Line 2
	Country
Contact person	Name Surname
Inquiry ID	Inquiry ID: 0001
Purchase order	-

Testing institute


Address	UAB Lidaris
	Saulėtekio al. 10
	10223 Vilnius
	Lithuania
Tester	Name Surname
Test date	01/01/2021
Sale order	SO0001
Test ID	-

Specimen

Name	Sample
Type	AR Coating (AR @ 1053 nm, AOI = 0 deg)
Dimensions	Ø25.4 x 6.0 mm
Packaging	Paper

TEST EQUIPMENT

Test setup

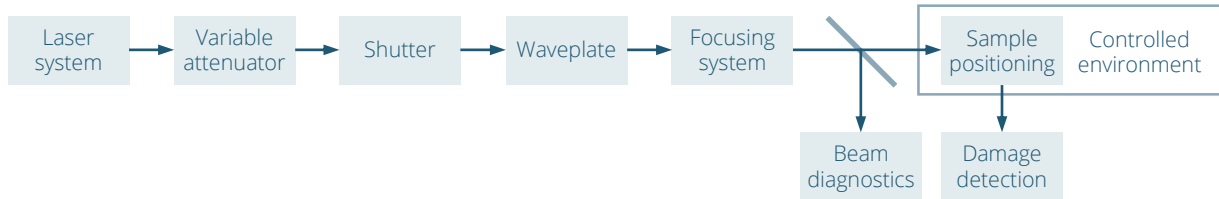

Laser and its parameters

Type	Q-switched, seeded Nd:YAG
Manufacturer	InnoLas Laser II
Model	SpitLight Hybrid
Central wavelength	1064.0 nm
Angle of incidence	0.0 deg
Polarization state	Linear
Pulse repetition frequency	100 Hz
Spatial beam profile in target plane	TEM00
Beam diameter in target plane ($1/e^2$)	$(222.1 \pm 3.5) \mu\text{m}$
Longitudinal pulse profile	Single longitudinal mode
Pulse duration (FWHM)	$(10.1 \pm 0.3) \text{ ns}$
Pulse to pulse energy stability (SD)	0.7 %

Energy/power meter

Manufacturer	Ophir
Model	PE50-DIF-C
Calibration due date	2021-06-01

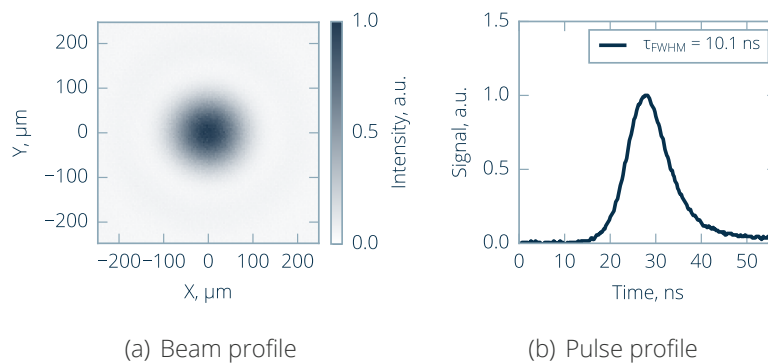


Figure 1. Laser parameters used for measurements.

TEST SPECIFICATION

Definitions and test description

Laser-induced damage (LID) is defined as any permanent laser radiation induced change in the characteristics of the surface/bulk of the specimen which can be observed by an inspection technique and at a sensitivity related to the intended operation of the product concerned. Laser-induced damage threshold (LIDT) is defined as the highest quantity of laser radiation incident upon the optical component for which the extrapolated probability of damage is zero. ¹

R-on-1 test uses multiple pulses when irradiating single site of the sample. Starting from very low values fluence is constantly increased step by step until damage is reached.

Test sites

Number of sites	10
Arrangement of sites	Hexagonal
Minimum distance between sites	900 µm
Start fluence	4.0
Fluence step	4.0
Pulses per fluence level	100

Analysis information

Online detection	Scattered light diode
Offline detection	Nomarski microscope
Software version	3d30819 - a465db1

Test environment

Environment	Air
Cleanroom class (ISO 14644-1)	ISO7
Pressure	1 bar
Temperature	22.5 - 22.5 C
Humidity	33.0 - 33.1 %

Sample preparation

Storage before test	Normal laboratory conditions
Dust blow-off	Compressed air
Cleaning	Butyl Acetate

¹ISO 21254-1:2011: Lasers and laser-related equipment - Test methods for laser-induced damage threshold - Part 1: Definitions and general principles, International Organization for Standardization, Geneva, Switzerland (2011)

LIDT TEST RESULTS

R-ON-1 LIDT

Table 1: Evaluated R-on-1 LIDT for sample Sample.

Test mode	Threshold
R(100)-on-1	$42.4^{+5.0}_{-4.7} \text{ J/cm}^2$

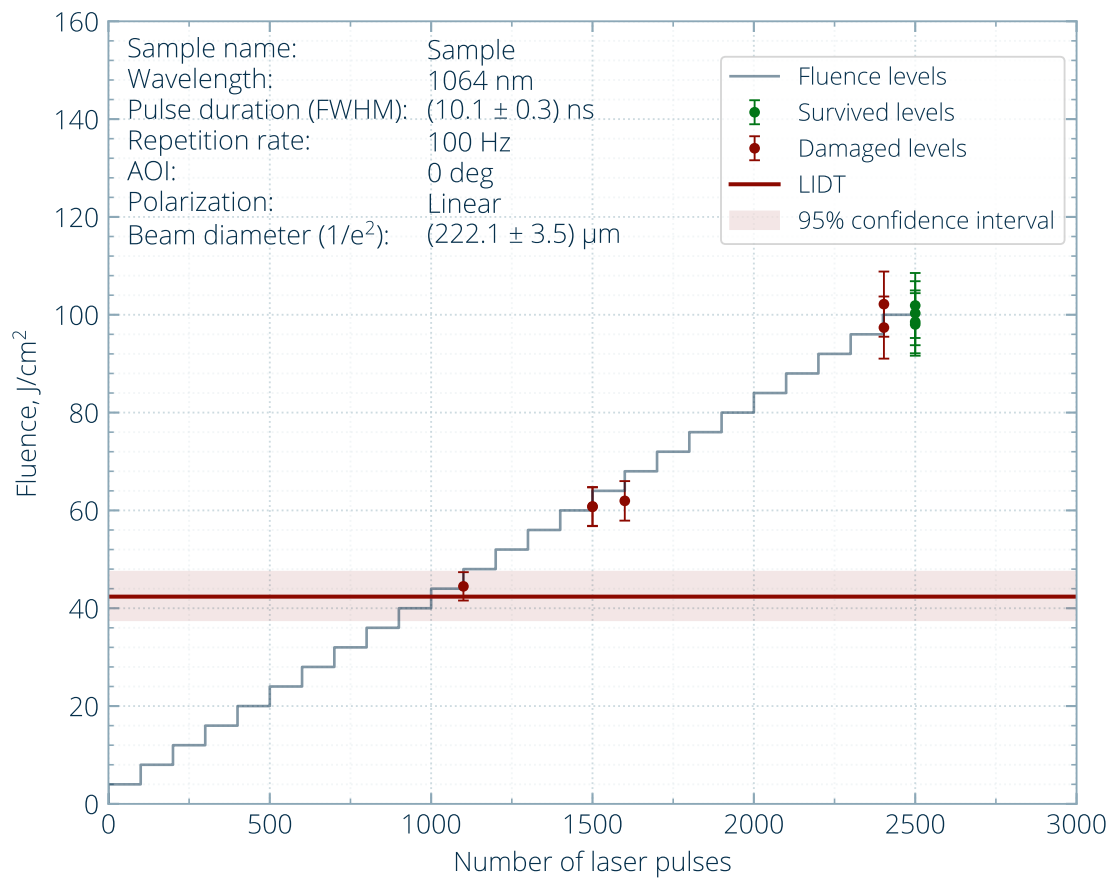


Figure 2. R-on-1 test results.

TEST POINTS

Table 2: R-on-1 damaged test points for sample Sample.

Test mode	Damaging level	Mean fluence	Number of pulses
R(100)-on-1	15	60.7 $^{+4.0}_{-4.0}$ J/cm ²	100
R(100)-on-1	25	102.2 $^{+6.7}_{-6.7}$ J/cm ²	3
R(100)-on-1	11	44.5 $^{+2.9}_{-2.9}$ J/cm ²	100
R(100)-on-1	16	62.0 $^{+4.0}_{-4.0}$ J/cm ²	100
R(100)-on-1	25	97.4 $^{+6.4}_{-6.4}$ J/cm ²	3
R(100)-on-1	15	60.8 $^{+4.0}_{-4.0}$ J/cm ²	100
R(100)-on-1	survived	98.0 $^{+6.4}_{-6.4}$ J/cm ²	-
R(100)-on-1	survived	98.6 $^{+6.4}_{-6.4}$ J/cm ²	-
R(100)-on-1	survived	101.9 $^{+6.6}_{-6.6}$ J/cm ²	-
R(100)-on-1	survived	100.3 $^{+6.5}_{-6.5}$ J/cm ²	-

TYPICAL DAMAGE MORPHOLOGY

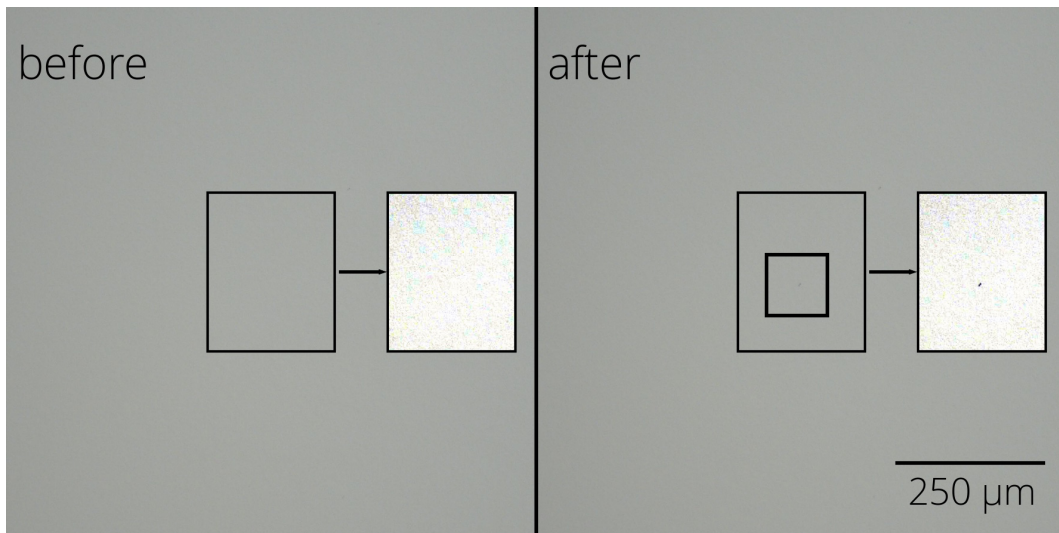


Figure 3. Typical damage morphology: fluence 44.5 J/cm^2 , damage after 100 pulse(s) in fluence level. High contrast image.



Figure 4. Typical damage morphology: fluence 60.7 J/cm^2 , damage after 100 pulse(s) in fluence level.



Figure 5. Typical damage morphology: fluence 60.8 J/cm^2 , damage after 100 pulse(s) in fluence level.