

SO0001



LASER-INDUCED DAMAGE THRESHOLD (LIDT) MEASUREMENT REPORT

LIDT ISO PASS/FAIL TEST
PROCEDURE

SAMPLE: SAMPLE

Request from

Address

Company

Address Line 1

Address Line 2

Country

Contact person

Name Surname

Inquiry ID

Inquiry ID: 0001

Purchase order

-

Testing institute

Address

UAB Lidaris

Saulėtekio al. 10

10223 Vilnius

Lithuania

Tester

Name Surname

Test date

01/01/2025

Sale order

SO0001

Test ID

-

Specimen

Name

Sample

Front surface (S1)

AR Coating (AR@1064)

Rear surface (S2)

Uncoated

Dimensions


Ø25.0 x 2.0 mm

Packaging

Plastic box

TEST EQUIPMENT

Test setup

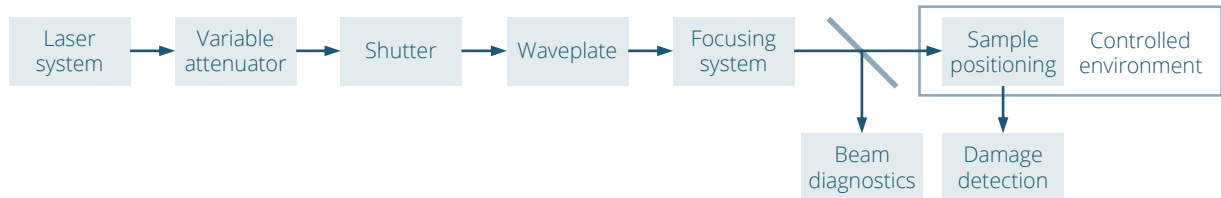

Laser and its parameters

Type	Q-switched, seeded Nd:YAG
Manufacturer	InnoLas Laser II
Model	SpitLight Hybrid
Central wavelength	1064.0 nm
Angle of incidence	0.0 deg
Polarization state	Linear
Pulse repetition frequency	20 Hz
Spatial beam profile in target plane	TEM00
Beam diameter in target plane ($1/e^2$)	$(1001.7 \pm 6.2) \mu\text{m}$
Longitudinal pulse profile	Single longitudinal mode
Pulse duration (FWHM)	$(10.0 \pm 0.3) \text{ ns}$
Pulse to pulse energy stability (SD)	0.6 %

Energy/power meter

Manufacturer	Ophir
Model	PE50-DIF-C
Calibration due date	2027-12-31

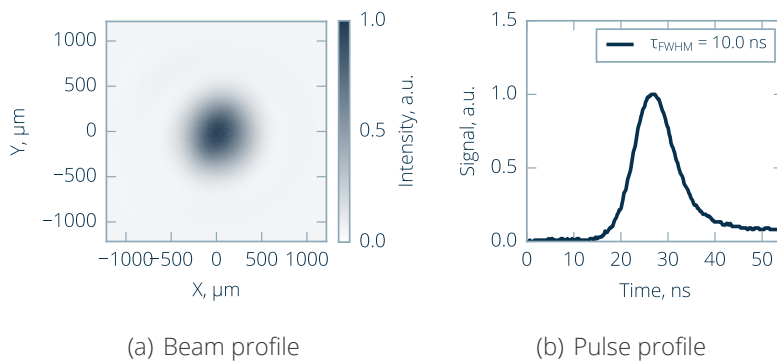


Figure 1. Laser parameters used for measurements.

TEST SPECIFICATION

Definitions and test description

Laser-induced damage (LID) is defined as any permanent laser radiation induced change in the characteristics of the surface/bulk of the specimen which can be observed by an inspection technique and at a sensitivity related to the intended operation of the product concerned. Laser-induced damage threshold (LIDT) is defined as the highest quantity of laser radiation incident upon the optical component for which the extrapolated probability of damage is zero.

¹

Intensity handling capability of the sample is investigated by performing a standardized test procedure.²

Test sites

Assurance value	1 GW/cm ²
Number of sites	10
Arrangement of sites	Hexagonal
Minimum distance between sites	3000 µm
Maximum pulses per site	1000

Analysis information

Online detection	Scattered light diode
Offline detection	Nomarski microscope
Software version	f6ced89e

Test environment

Environment	Air
Cleanroom class (ISO 14644-1)	ISO7
Pressure	1 bar
Temperature	22.3 - 22.9 C
Humidity	53.2 - 54.6 %

Sample preparation

Storage before test	Normal laboratory conditions
Dust blow-off	Canned air
Cleaning	None

¹ISO 21254-1:2011: Lasers and laser-related equipment - Test methods for laser-induced damage threshold - Part 1: Definitions and general principles, International Organization for Standardization, Geneva, Switzerland (2011)

²ISO 21254-3:2011: Lasers and laser-related equipment - Test methods for laser-induced damage threshold - Part 3: Assurance of laser power (energy) handling capabilities, International Organization for Standardization, Geneva, Switzerland (2011)

LIDT TEST RESULTS

INTENSITY HANDLING CAPABILITY

Table 1: Intensity handling capability of sample Sample.

Intensity	Pulses	Result
$(996 \pm 29) \text{ MW/cm}^2$	1000	Failed

TYPICAL DAMAGE MORPHOLOGY



Figure 2. Test site after 1000 pulse(s).



Figure 3. Test site after 1000 pulse(s).